TECHNICAL REPORT
NATICK/TR-96/004

AD_____

# EXPERIMENTAL UNCERTAINTY IN THIRD-ORDER SUSCEPTIBILITY AND MOLECULAR SECOND HYPERPOLARIZABILITY MEASUREMENTS OBTAINED WITH DEGENERATE FOUR-WAVE MIXING

By

**Brian R. Kimball**
and
**Joseph F. Roach**

December 1995

Final Report

March 1994 - November 1994

Approved for public release, distribution unlimited

## UNITED STATES ARMY SOLDIER SYSTEMS COMMAND
## NATICK RESEARCH, DEVELOPMENT AND ENGINEERING CENTER
## NATICK, MASSACHUSETTS 01760-5020

## DISCLAIMERS

The findings contained in this report are not to

be construed as an official Department of the Army

position unless so designated by other authorized

documents.

Citation of trade names in this report does not

constitute an official endorsement or approval of

the use of such items.

## DESTRUCTION NOTICE

For Classified Documents:

Follow the procedures in DoD 5200.22-M, Industrial

Security Manual, Section II-19 or DoD 5200.1-R,

Information Security Program Regulation, Chapter IX.

For Unclassified/Limited Distribution Documents:

Destroy by any method that prevents disclosure of

contents or reconstruction of the document.

# REPORT DOCUMENTATION PAGE

| 1. AGENCY USE ONLY (Leave blank) | 2. REPORT DATE | 3. REPORT TYPE AND DATES COVERED |
|---|---|---|
| | December 1995 | FINAL - March 1994 - November 1994 |

**4. TITLE AND SUBTITLE**
Experimental Uncertainty in Third-Order
Susceptibility and Molecular Second Hyperpolarizability
Measurements Obtained with Degenerate Four-Wave Mixing

**5. FUNDING NUMBERS**
AgC: TB1089PE

PR: 1L1AH980

TA: CAOAOO

**6. AUTHOR(S)**
Brian R. Kimball and Joseph F. Roach

**7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES)**
U.S. Army Soldier Systems Command
Natick RD&E Center
Kansas St. ATTN: AMSSC-YSD
Natick, MA 01760-5020

**8. PERFORMING ORGANIZATION REPORT NUMBER**
NATICK/TR-96/004

**9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES)**

**10. SPONSORING / MONITORING AGENCY REPORT NUMBER**

**11. SUPPLEMENTARY NOTES**

**12a. DISTRIBUTION / AVAILABILITY STATEMENT**

Approved for public release, distribution unlimited

**12b. DISTRIBUTION CODE**

**13. ABSTRACT (Maximum 200 words)**

An uncertainty analysis is performed on a degenerate four-wave mixing scheme used in the determination of the third-order susceptibility and molecular second hyperpolarizability of nonlinear optical materials. Equations are derived based on the root-sum-squares method, which accounts for uncertainty in all applicable experimental parameters. These expressions are incorporated into a computer program, which is used to investigate absolute and relative uncertainties as well as the sensitivity of overall system accuracy to individual parameters. Conclusions are drawn based on the results of the analysis.

**14. SUBJECT TERMS**
THIRD-ORDER SUSCEPTIBILITY   THIRD-ORDER NONLINEARITIES
NONLINEAR OPTICAL MATERIALS   FOUR-WAVE MIXING   OPTICAL NONLINEARITY
DEGENERATE FOUR-WAVE MIXING   STATISTICAL ANALYSIS   LASER EYE PROTECTION
UNCERTAINTY ANALYSIS

**15. NUMBER OF PAGES**
45

**16. PRICE CODE**

| 17. SECURITY CLASSIFICATION OF REPORT | 18. SECURITY CLASSIFICATION OF THIS PAGE | 19. SECURITY CLASSIFICATION OF ABSTRACT | 20. LIMITATION OF ABSTRACT |
|---|---|---|---|
| Unclassified | Unclassified | Unclassified | |

# TABLE OF CONTENTS

# LIST OF FIGURES

# LIST OF TABLES

## PREFACE

This report summarizes the development and application of an analysis of the uncertainty in third-order susceptibility and second hyperpolarizability measurements obtained experimentally with degenerate four-wave mixing. This work is being done under the project Laser Eye Protection, 5325006CA0A00, administered by the Technology Application Branch, Fiber and Polymer Science Division, Science and Technology Directorate, U.S. Army Soldier Systems Command, Natick Research, Development, and Engineering Center.

All experiments were performed at the Technology Application Branch, at the Natick Research, Development, and Engineering Center (Natick). The citation of trade names in this report does not constitute official endorsement or approval of use of an item.

# EXPERIMENTAL UNCERTAINTY IN THIRD-ORDER SUSCEPTIBILITY
# AND MOLECULAR SECOND HYPERPOLARIZABILITY MEASUREMENTS
# OBTAINED WITH DEGENERATE FOUR WAVE MIXING

## INTRODUCTION

Third-order susceptibility and molecular second hyperpolarizability measurements are currently performed with degenerate four-wave mixing (DFWM). Experimental values obtained by this technique have been reported with estimated confidence intervals. This report describes an uncertainty analysis that can be used to 1) better define experimental uncertainties, 2) add some insight into the degree to which individual experimental parameters affect overall system accuracy, and 3) validate comparisons of experimental $\chi^{(3)}$ and $\langle \gamma \rangle$ values for various compounds to confirm the significance of any observed variations in nonlinear response, as in the study of trends.

The DFWM system described here utilizes a backward-beam geometry where two strong collinear pump beams, propagating in opposite directions, interact at the sample with a third less-intense probe beam to create a fourth nonlinear optical phase conjugate beam. The intensity of the conjugate signal is proportional to the square of the $\chi^{(3)}$ of the sample under study. The signal is measured with a silicon photodiode and oscilloscope. It is then compared to a similar signal obtained from a carbon disulfide standard under identical conditions using the expression

$$\frac{\chi^{(3)}{}_{sample}}{\chi^{(3)}{}_{CS_2}} = \left(\frac{n_{sample}}{n_{CS_2}}\right)^2 \frac{d\alpha}{1-e^{-\alpha d}} e^{\alpha d/2} \left(\frac{I_{sample}}{I_{CS_2}}\right)^{1/2} \frac{d_{CS_2}}{d_{sample}} \cdots \tag{1}$$

where $n$ is the index of refraction, $\alpha$ is the linear absorption coefficient, $d$ is the length of the sample and $I$ is the measured signal of the phase conjugate beam. This approach eliminates the need of obtaining absolute irradiance measurements for each of the additional three beams used in the DFWM setup.[1]

The relationship between the molecular second hyperpolarizability $\langle \gamma \rangle$ and the third-order macroscopic susceptibility of the solute is given by the expression

$$\langle \gamma \rangle = \frac{\chi^{(3)}}{L^4 N} \tag{2}$$

where $N$ is the number density of molecules per mL and

$$L = \frac{n^2 + 2}{3}.$$  (3)

It is generally assumed that the conjugate signal is due to a combination of third-order nonlinearities in both the solvent and solute and that for a solution of noninteracting particles the relationship is additive:[1]

$$\chi^3_{solution} = L^4 [N_{solvent} \gamma_{solvent} + N_{solute} \gamma_{solute}] \cdots$$  (4)

The $\chi^{(3)}_{solution}$ is obtained experimentally with Eq. 1. For nonsaturated solutions

$$N_{solute} = \frac{A C}{M}$$  (5)

where $A$ is Avogadro's number, $M$ is the molecular weight of the solute, and $C$ is the concentration. Making appropriate substitutions of Eqs. 2 and 5 into Eq. 4, the following expression is obtained:

$$\chi^3_{solution} = \chi^3_{solvent} + (L^4 \gamma_{solute} A/M) C.$$  (6)

By evaluating Eq. 1 for a series of dilute solutions and plotting the results versus respective concentration, a straight line is obtained. A least-squares approximation is then applied to the data from which one obtains $\chi^{(3)}_{solvent}$ from the y-intercept and $\gamma_{solute}$ from the slope. The $\chi^{(3)}_{solute}$ is then obtained from Eq. 2.

# DERIVATION OF UNCERTAINTY EQUATIONS

If it is assumed that the uncertainties $(W_1, W_2, \ldots, W_n)$ in the independent variables $(X_1, X_2, \ldots, X_n)$ are all given with the same probability, then the uncertainty $(W_R)$ in the dependent variable $(R)$ is given by the expression

$$W_R = \left[ \left( \frac{(\partial R)}{\partial X_1} W_1 \right)^2 + \left( \frac{(\partial R)}{\partial X_2} W_2 \right)^2 + \ldots + \left( \frac{(\partial R)}{\partial X_N} W_N \right)^2 \right]^{1/2}. \tag{7}$$

By inserting Eq. 1 into Eq. 7 a probable estimate of the uncertainty in experimentally determined $\chi^{(3)}{}_{sample}$ is obtained:

$$W_{\chi^{(3)}{}_s} = \left[ \left( \frac{\partial \chi^{(3)}{}_s}{\partial \chi^{(3)}{}_R} W_{\chi^3} \right)^2 + \left( \frac{\partial \chi^{(3)}{}_s}{\partial I_s} W_{I_s} \right)^2 + \left( \frac{\partial \chi^{(3)}{}_s}{\partial I_R} W_{I_R} \right)^2 + \left( \frac{\partial \chi^{(3)}{}_s}{\partial n_s} W_{n_s} \right)^2 + \right.$$
$$\left. + \left( \frac{\partial \chi^{(3)}{}_s}{\partial n_R} W_{n_R} \right)^2 + \left( \frac{\partial \chi^{(3)}{}_s}{\partial d_R} W_{d_R} \right)^2 + \left( \frac{\partial \chi^{(3)}{}_s}{\partial d_s} W_{d_s} \right)^2 + \left( \frac{\partial \chi^3{}^{(3)}{}_s}{\partial \alpha} W_\alpha \right)^2 \right]^{1/2}, \tag{8}$$

where

$$\frac{\partial \chi^{(3)}{}_s}{\partial \chi^{(3)}{}_R} = \left( \frac{I_s}{I_R} \right)^{1/2} \left( \frac{n_s}{n_R} \right)^2 \left( \frac{d_R}{d_s} \right) \frac{\alpha L}{(1 - e^{-\alpha L})} e^{\alpha L/2}, \tag{9}$$

$$\frac{\partial \chi^{(3)}{}_s}{\partial I_s} = \frac{\chi^{(3)}{}_R}{2\sqrt{I_s I_R}} \left( \frac{n_s}{n_R} \right)^2 \left( \frac{d_R}{d_s} \right) \frac{\alpha L}{(1 - e^{-\alpha L})} e^{\alpha L/2}, \tag{10}$$

$$\frac{\partial \chi^{(3)}{}_s}{\partial I_R} = \frac{-\chi^{(3)}{}_R}{2} \frac{(I_s)^{1/2}}{(I_R)^{3/2}} \left( \frac{n_s}{n_R} \right)^2 \left( \frac{d_R}{d_s} \right) \frac{\alpha L}{(1 - e^{-\alpha L})} e^{\alpha L/2}, \tag{11}$$

$$\frac{\partial \chi^{(3)}{}_s}{\partial n_s} = \chi^{(3)}{}_R \left( \frac{I_s}{I_R} \right)^{1/2} \left( \frac{2 n_s}{n_R^2} \right) \left( \frac{d_R}{d_s} \right) \frac{\alpha L}{(1 - e^{-\alpha L})} e^{\alpha L/2}, \tag{12}$$

$$\frac{\partial \chi^{(3)}{}_s}{\partial n_R} = \chi^{(3)}{}_R \left( \frac{I_s}{I_R} \right)^{1/2} \left( \frac{-2 n_s^2}{n_R^3} \right) \left( \frac{d_R}{d_s} \right) \frac{\alpha L}{(1 - e^{-\alpha L})} e^{\alpha L/2}, \tag{13}$$

3

$$\frac{\partial \chi^{(3)}{}_s}{\partial d_R} = \chi^{3)}{}_R \left(\frac{I_s}{I_R}\right)^{1/2} \left(\frac{n_s}{n_R}\right)^2 \left(\frac{1}{d_s}\right) \frac{\alpha L}{(1-e^{-\alpha L})} e^{\alpha L/2}, \tag{14}$$

$$\frac{\partial \chi^{(3)}{}_s}{\partial d_s} = \chi^{(3)}{}_R \left(\frac{I_s}{I_R}\right) \left(\frac{n_s}{n_R}\right)^2 \left(\frac{-d_R}{d_s^2}\right) \frac{\alpha L}{(1-e^{-\alpha L})} e^{\alpha L/2}, \tag{15}$$

and

$$\frac{\partial \chi^{(3)}{}_s}{\partial \alpha} = \chi^{(3)}{}_R \left(\frac{I_s}{I_R}\right)^{1/2} \left(\frac{n_s}{n_R}\right)^2 \left(\frac{d_R}{d_s}\right) \frac{(1-e^{-\alpha L})\left[L\left(\frac{\alpha L}{2}+e^{\alpha L/2}\right)\right]-\alpha L^2 e^{-\alpha L/2}}{(1-e^{-\alpha L})^2}. \tag{16}$$

Similarly, for the uncertainty in $\langle \gamma \rangle$, Eq. 2 is applied to Eq. 7 to obtain:

$$W_\gamma = \left[\left(\frac{\partial \gamma}{\partial \chi^{(3)}} W_{\chi^{(3)}}\right)^2 + \left(\frac{\partial \gamma}{\partial M} W_M\right)^2 + \left(\frac{\partial \gamma}{\partial L} W_L\right)^2 + \left(\frac{\partial \gamma}{\partial A} W_A\right)^2\right]^{1/2}, \tag{17}$$

where

$$\frac{\partial \gamma}{\partial \chi^{(3)}} = \frac{M}{L^4 A}, \tag{18}$$

$$\frac{\partial \gamma}{\partial M} = \frac{\chi^{(3)}}{L^4 A}, \tag{19}$$

$$\frac{\partial \gamma}{\partial L} = \frac{-4\chi^{(3)} M}{L^5 A}, \tag{20}$$

and

$$\frac{\partial \gamma}{\partial A} = 0 \quad (assumed). \tag{21}$$

In order to evaluate Eq. 8, absolute error values are required for $\chi^{(3)}{}_R$, $I_s$, $I_R$, $n_s$, $n_R$, $d_R$, $d_s$, and $\alpha$. These can all be determined directly through

4

experimental considerations or can be given assumed values. For Eq. 17 error values for $M$, $\chi^{(3)}$ (solute), and $L$ must be obtained. Additional calculations must be performed to obtain estimates for the uncertainty in $\chi^{(3)}$ (solute), and $L$. For $W_L$, Eqs 3 and 7 are combined:

$$W_L = \left[ \left( \frac{\partial L}{\partial n_s} W_{n_s} \right)^2 \right]^{1/2} , \tag{22}$$

where

$$\frac{\partial L}{\partial n_s} = \frac{2n_s}{3} . \tag{23}$$

For the uncertainty in $\chi^{(3)}$, Eq. 6 is first written in the form:

$$\chi^{(3)}_{slt} = \frac{\left( \chi^{(3)}_{s} - \chi^{(3)}_{slv} \right) (1000)}{C} . \tag{24}$$

The factor of 1000 is included as a dimensional constant. Applying Eq. 7:

$$W_{\chi^{(3)}_{slt}} = \left[ \left( \frac{\partial \chi^{(3)}_{slt}}{\partial \chi^{(3)}_{s}} W_{\chi^{(3)}_{s}} \right)^2 + \left( \frac{\partial \chi^{(3)}_{slt}}{\partial \chi^{(3)}_{slv}} W_{\chi^{(3)}_{slv}} \right)^2 + \left( \frac{\partial \chi^{(3)}_{slt}}{\partial C} W_C \right)^2 \right]^{1/2} , \tag{25}$$

where

$$\frac{\partial \chi^3_{slt}}{\partial \chi^3_{s}} = \frac{1000}{C} , \tag{26}$$

$$\frac{\partial \chi^3_{slt}}{\partial \chi^3_{slv}} = \frac{-1000}{C} , \tag{27}$$

and

$$\frac{\partial \chi^3_{slt}}{\partial \chi^3_{slv}} = 1000 \left( \frac{\chi^{(3)}_{s} - \chi^{(3)}_{slv}}{C^2} \right) . \tag{28}$$

5

The value of $W_C$ depends upon the method with which the solutions are prepared. The technique currently being used relies on accurate weight measurements to determine the solution concentration. Briefly, an initial concentration $(C_i)$ is prepared using a precision balance for the solute and a volumetric flask for the solvent. For each run a portion of the solution is used. After each run the mass of the remaining solution is determined $(m_f)$. The flask is again filled and weighed to obtain the initial weight of the next run $(m_n)$. Using the following expression the new concentration is obtained (see Appendix A for derivation):

$$C_n = C_i \frac{m_f}{m_n}. \tag{29}$$

Advantages of this technique include ease of weight measurements, a reduction in waste solvent, and high overall accuracy. To obtain $W_C$ we evaluate the following equation:

$$W_{C_n} = \left[ \left( \frac{\partial C_n}{\partial C_i} W_{C_i} \right)^2 + \left( \frac{\partial C_n}{\partial m_f} W_{m_f} \right)^2 + \left( \frac{\partial C_n}{\partial m_n} W_{m_n} \right)^2 \right]^{1/2}, \tag{30}$$

where

$$\frac{\partial C_n}{\partial C_i} = \frac{m_f}{m_n}, \tag{31}$$

$$\frac{\partial C_n}{\partial m_f} = \frac{C_i}{m_n}, \tag{32}$$

and

$$\frac{\partial C_n}{\partial m_n} = \frac{-C_i m_f}{m_n^2}. \tag{33}$$

In order to evaluate Eq. 30 a value for $W_{C_i}$ must be estimated. Beginning with the expression

$$C_i = \frac{m_i}{V_i}, \tag{34}$$

6

where $m_i$ is the initial weight and $V_i$ is the initial volume, we must evaluate the following equation:

$$W_{C_i} = \left[ \left( \frac{\partial C_i}{\partial m_i} W_{m_i} \right)^2 + \left( \frac{\partial C_i}{\partial V_i} W_{V_i} \right)^2 \right]^{1/2}, \tag{35}$$

where

$$\frac{\partial C_i}{\partial m_i} = \frac{1}{V_i}, \tag{36}$$

and

$$\frac{\partial C_i}{\partial V_i} = \frac{-m_i}{V_i^2}. \tag{37}$$

These expressions have been incorporated into a computer program (Appendix B) which calculates $\chi^{(3)}_{solution}$, $\chi^{(3)}_{solute}$, and $\langle \gamma \rangle_{solute}$ and the uncertainties associated with each of these values.

## EXPERIMENTAL-PARAMETER SENSITIVITY

In order to evaluate the uncertainty equations that were derived in the previous section, values are assumed for the absolute errors of the independent variables. These are given as percent errors in Table 1.

Table 1. Assumed percent errors for experimental parameters

| Parameter | Assumed Percent Error |
|---|---|
| $\chi^{(3)}{}_{CS2}$ | 0% |
| $I_{solution}$ | 5% |
| $I_{CS2}$ | 5% |
| $n_{solution}$ | 1% |
| $n_{CS2}$ | 0.1% |
| $d_{sample}$ | 0.1% |
| $d_{CS2}$ | 0.1% |
| $\alpha_{solution}$ | 0.08% |
| $M_{solute}$ | 0.1% |
| $mass_{solution}$ | 1% |
| $volume_{solution}$ | 1% |

It is assumed that an exact value for $\chi^{(3)}{}_{CS2}$ is known. Uncertainties in intensity measurements are based on an estimate of the readability of the oscilloscope used in the evaluations. The index of refraction for $CS_2$ is considered more accurate than that of the sample because it is assumed that $n_{solution} = n_{solvent}$, and additional error is allowed here. Percent errors given for the cell thicknesses $d_{sample}$ and $d_{CS2}$ are manufacturer stated tolerances. Mass and volume tolerances are based on scale readabilities.

Absolute errors for solution concentrations are calculated using Eq. 30. These will slightly increase with each new solution that is prepared. For example, for an initial concentration of 1 mg/mL, where 0.005 g of solute is dissolved in 5 mL of solvent with tolerances of ±0.0001 g and ± 0.05 mL, respectively, Eq. 35 gives an uncertainty of 0.00002 g/mL or 2.2% for the initial concentration. This value is then used as input into Eq. 30 to obtain the uncertainty in the following, more dilute solution. Table 2 shows an example in which each consecutive concentration is half the previous concentration. New concentrations ($C_n$) are calculated at the end of each run using the mass measurements shown for that run and Eq. 29. Absolute uncertainties ($W_{Cn}$) are predicted with Eq. 30 and percent errors are also shown for each run.

Table 2. Uncertainty in concentration measurements for a standard run.

| $c_i$ (g/mL) | $m_i$ (g) | $m_f$ (g) | $m_n$ (g) | $c_n$ (g/mL) | $W_{cn}$ (g/mL) | % Error |
|---|---|---|---|---|---|---|
| $1\times10^{-3}$ | 4.6 | 2.3 | 4.6 | $5\times10^{-4}$ | $1\times10^{-5}$ | 1% |
| $5\times10^{-4}$ | 4.6 | 2.3 | 4.6 | $2.5\times10^{-4}$ | $5\times10^{-6}$ | 1% |
| $2.5\times10^{-4}$ | 4.6 | 2.3 | 4.6 | $1.25\times10^{-4}$ | $4\times10^{-6}$ | 1.6% |
| $1.25\times10^{-4}$ | 4.6 | 2.3 | 4.6 | $6.25\times10^{-5}$ | $2\times10^{-6}$ | 1.6% |
| $6.25\times10^{-5}$ | 4.6 | 2.3 | 4.6 | $3.12\times10^{-5}$ | $1\times10^{-6}$ | 1.6% |

These values are used as input to program ERRCHI-3.BAS. Table 3 gives additional input for a representative run where the $\chi^{(3)}$ of zinc tetraphenyl tetrabenzporphyrin in tetrahydrafuran was evaluated.

Table 3. ERRCHI-3.BAS input data for experimental run of zinc tetraphenyl tetrabenzporphyrin in tetrahydrafuran.

| Variable | Input |
|---|---|
| $I_{solution}$ | 28000 |
| $I_{CS2}$ | 150000 |
| $\propto$ | 0.875 |
| $c_i$ | 0.00076 g/mL |
| $\chi^{(3)}_{solvent}$ | $2.4\times10^{-14}$ esu |
| $W_{\chi(3)solvent}$ | $9.7\times10^{-16}$ esu |
| M | 678 |
| weight | 0.0038 g |
| vol | 5 mL |

The following output was obtained for this run:

$\chi^{(3)}$ of solution = $1.45\times10^{-12}$
Uncertainty = $5.94\times10^{-14}$
Percent Error = 4%


$\chi^{(3)}$ of solute = $1.88\times10^{-9}$
Uncertainty = $7.85\times10^{-11}$
Percent Error = 4%

$\langle \gamma \rangle$ of solute = $6.3 \times 10^{-31}$

Uncertainty = $3.64 \times 10^{-32}$

Percent Error = 6%


Uncertainty in $\chi^{(3)}_{solution}$ due to:

$\quad$ $\chi^{(3)}_{CS2}$ = 0

$\quad$ Voltage reading for solution = $3.6 \times 10^{-14}$

$\quad$ Voltage reading for $CS_2$ = $3.6 \times 10^{-14}$

$\quad$ Solution refractive index = $2.9 \times 10^{-14}$

$\quad$ $CS_2$ refractive index = $2.9 \times 10^{-15}$

$\quad$ Solution cell thickness = $1.5 \times 10^{-15}$

$\quad$ $CS_2$ cell thickness = $1.5 \times 10^{-15}$

$\quad$ Sample absorption = $5.4 \times 10^{-16}$


Uncertainty in concentration due to:

$\quad$ Weight = 0.0076

$\quad$ Volume = 0.0076


Uncertainty in $\chi^{(3)}_{solute}$ due to:

$\quad$ $\chi^{(3)}_{solution}$ = $7.8 \times 10^{-11}$

$\quad$ $\chi^{(3)}_{solvent}$ = $1.3 \times 10^{-11}$

$\quad$ Concentration = $2.7 \times 10^{-11}$


Uncertainty in field factor due to:

$\quad$ Solution refractive index = 0.014


Uncertainty in $\langle \gamma \rangle$ due to:

$\quad$ $\chi^{(3)}_{solute}$ = $2.7 \times 10^{-32}$

$\quad$ Molecular weight = $6.3 \times 10^{-34}$

$\quad$ Field factor (L) = $2.5 \times 10^{-32}$


The value for $\chi^{(3)}_{solvent}$ and its corresponding uncertainty was obtained by first running the program at zero concentration. Uncertainties due to individual experimental parameters shown above are obtained from the product of the parameter sensitivity and its absolute uncertainty, for instance, from Eq. 7:

$$\frac{\partial R}{\partial X_1} W_1 . \tag{38}$$

10

These values show the relative degree to which single variables contribute to the overall uncertainty. For example, the greatest degree of uncertainty in the experimental value for $\chi^{(3)}_{solution}$ is due to oscilloscope voltage readings.

A similar output to that shown above is obtained for each concentration evaluated in the series. Each value of $\chi^{(3)}_{solution}$, $\chi^{(3)}_{solute}$, and $\langle\gamma\rangle$ will have an associated uncertainty based on the values of the experimental parameters unique to that run. The final values reported for $\chi^{(3)}_{solution}$, $\chi^{(3)}_{solute}$, and $\langle\gamma\rangle$ are obtained via a curve fitting technique while their respective uncertainties are obtained by taking the sample standard deviation of the individual uncertainties obtained for each run.

In some instances the input uncertainties given in Table 1 may vary; for example, in a case where the sample is in the form of a thin film, the thickness of which can only be approximated. With this in mind a series of plots were generated which show the change in the uncertainty of $\chi^{(3)}_{solute}$ and $\langle\gamma\rangle$ resulting from an increase in the uncertainty of a single variable. These are shown in Appendix C, Figs. C1-C21. In each plot the uncertainty in a single independent variable has been increased from 0% to 50% error while the uncertainty in the remaining independent variables has been kept constant at the current values.

The series of sensitivity plots for both $\chi^{(3)}_{solute}$ and $\langle\gamma\rangle$ are summarized in the following bar charts where the normalized average slope of each variable is shown. The charts show the relative degree to which a given variable is sensitive to changes in percent error. For example, the uncertainty in $\chi^{(3)}_{solute}$ is most sensitive to uncertainty in the refractive indices of both $CS_2$ and the solution while accuracy in determining the linear absorption of the sample has a minimal effect.

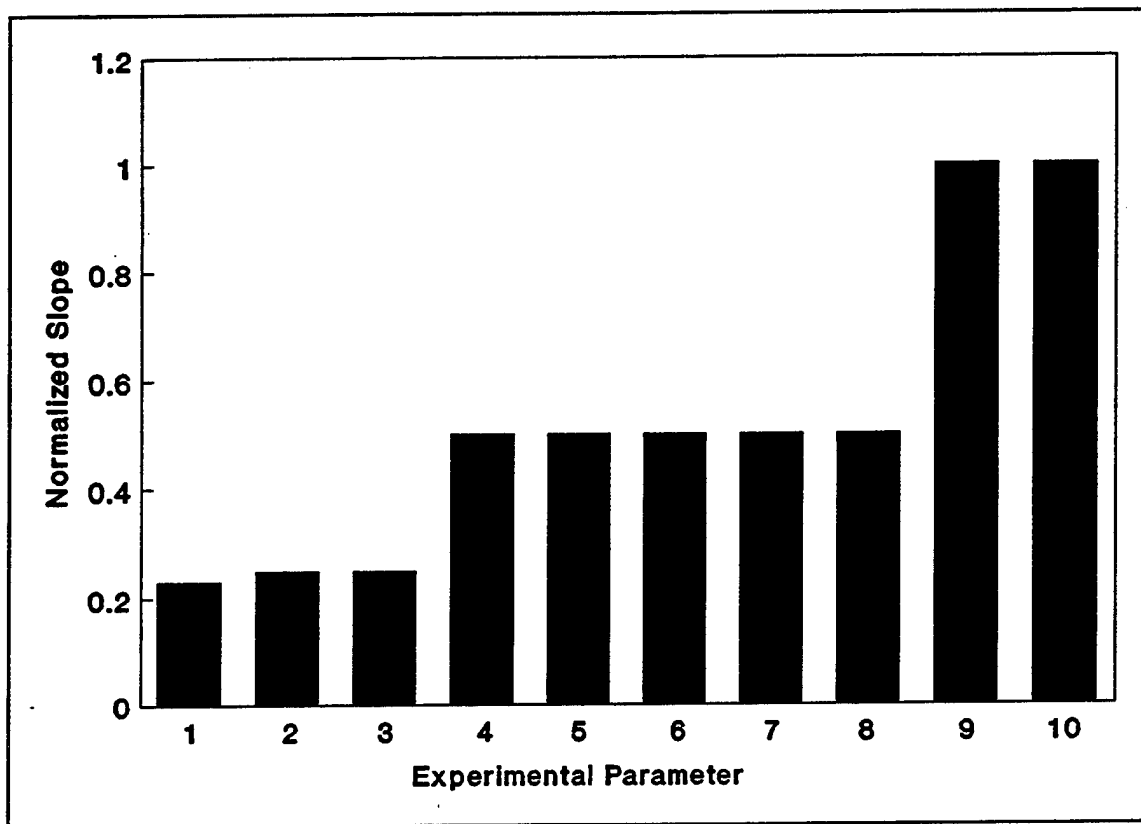Fig. 1. Normalized average slopes of parameter sensitivity
curves for $\chi^{(3)}_{solute}$.

Parameters shown in Fig. 1:

| | |
|---|---|
| 1 -- Sample absorption | 6 -- $CS_2$ thickness |
| 2 -- $I_{solution}$ | 7 -- Sample mass |
| 3 -- $I_{CS2}$ | 8 -- Sample volume |
| 4 -- $\chi^{(3)}_{CS2}$ | 9 -- $n_{CS2}$ |
| 5 -- Sample thickness | 10-- $n_{solution}$ |

Figure 2 shows that $\langle\gamma\rangle$ is also most sensitive to uncertainty in the refractive indices of $CS_2$ and sample solution. The increased dependence on $n_{solution}$ is due to its presence in the local field factor (Equation 3).
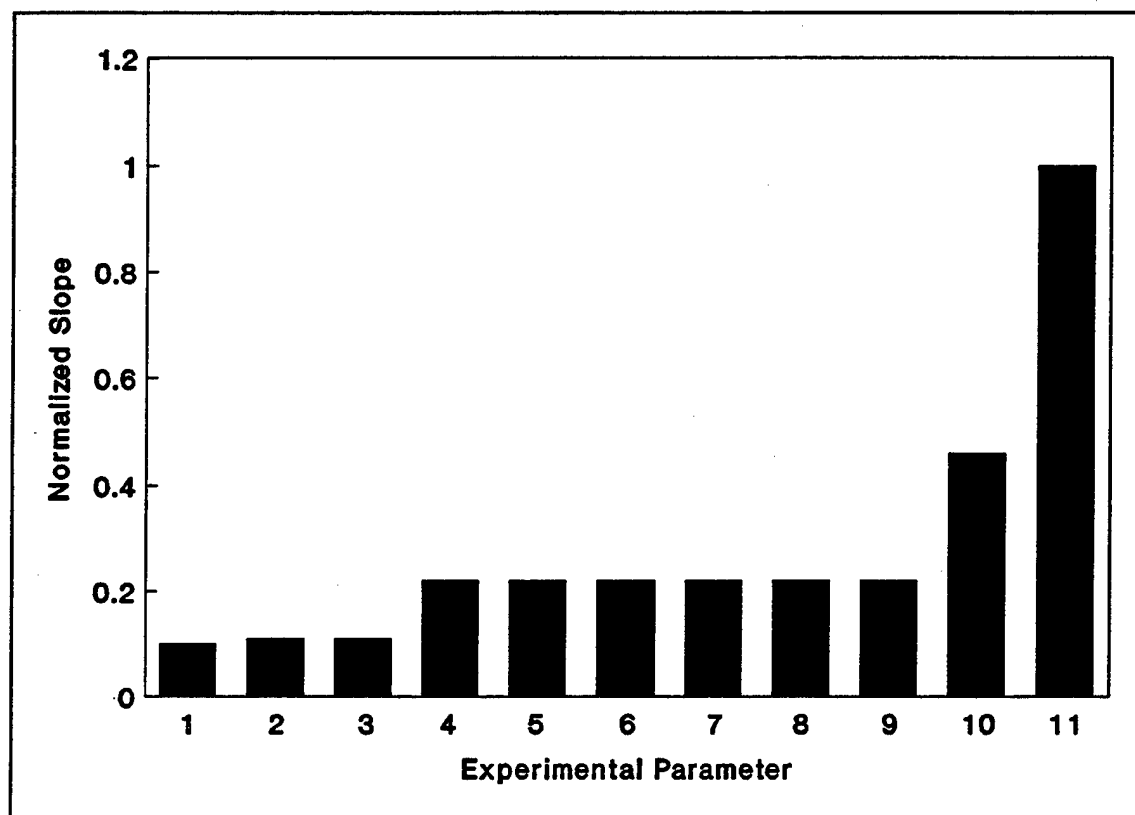
Fig. 2. Normalized average slopes of parameter sensitivity curves for $\langle \gamma \rangle$.

Parameters shown in Fig. 2:

1 -- Sample absorption
2 -- $I_{solution}$
3 -- $I_{CS2}$
4 -- $\chi^{(3)}_{CS2}$
5 -- Sample thickness
6 -- $CS_2$ thickness

7 -- Molecular weight
8 -- Sample mass
9 -- Sample volume
10-- $n_{CS2}$
11-- $n_{solution}$

A sampling of eight compounds evaluated for $\chi^{(3)}$ and $\langle\gamma\rangle$ reveals average $\chi^{(3)}$ and $\langle\gamma\rangle$ uncertainties of 8% and 9%, respectively, with values ranging from 6% to 10% for $\chi^{(3)}$ and 6% to 12% for $\langle\gamma\rangle$. In general, the lowest percent error is attributable to the highest voltage signal. Higher $\chi^{(3)}$ and $\langle\gamma\rangle$ values have higher associated phase-conjugate voltage readings and, therefore, lower percent uncertainties. For example, a material with a $\chi^{(3)}$ in the area of $10^{-9}$ will have a percent uncertainty of about 7% whereas a $\chi^{(3)}$ of $10^{-13}$ can have an uncertainty as high as 40%.

Table 4 shows the results obtained for zinc tetraphenyl tetrabenzporphyrin in tetrahydrafuran. It can be seen from these data that while the absolute uncertainty varies with concentration, the percent uncertainty remains relatively constant.

Table 4. Experimental results for zinc tetraphenyl tetrabenzporphyrin in tetrahydrafuran.

| $C$ (g/mL) | $\chi^{(3)}_{solution}$ ($\times 10^{-13}$ esu) | | | $\chi^{(3)}_{solute}$ ($\times 10^{-10}$ esu) | | | $\langle\gamma\rangle$ ($\times 10^{-31}$ esu) | | |
|---|---|---|---|---|---|---|---|---|---|
| 0.00216 | 43.7 | ±1.78 | (4%) | 20.1 | ±0.82 | (4%) | 6.66 | ±0.38 | (6%) |
| 0.00076 | 14.5 | ±0.59 | (4%) | 18.8 | ±0.78 | (4%) | 6.26 | ±0.36 | (6%) |
| 0.00038 | 9.57 | ±0.39 | (4%) | 24.5 | ±1.04 | (4%) | 8.12 | ±0.48 | (6%) |
| 0.00019 | 6.34 | ±0.25 | (4%) | 32.1 | ±1.44 | (4%) | 10.6 | ±0.64 | (6%) |
| 0.00010 | 2.31 | ±0.09 | (4%) | 21.2 | ±1.14 | (5%) | 7.03 | ±0.48 | (7%) |
| 0 | 0.24 | ±0.01 | (4%) | -- | -- | | -- | -- | |

Figure 3 shows the curve fit data from Table 4 where $\chi^{(3)}_{solute}$ versus concentration is shown. The straight line is obtained by plotting Eq. 24 with $\chi^{(3)}_{solvent} = 2.4 \times 10^{-14}$ esu, $\chi^{(3)}_{solute} = 2.0 \times 10^{-9}$ esu, and the concentrations shown in Table 4. Specific values for $\chi^{(3)}_{solution}$ are compared in Table 5 to experimental values obtained from Table 4. Percent errors given in Table 5 are calculated with the assumption that the curve-fit values are the more correct. It is generally expected that experimental deviations from the curve-fit line will be within one or two standard deviations as given in Table 4, or at most about 10%. Absolute errors shown in Table 5, in two cases, are outside predicted uncertainty. It is currently believed that these relatively large percent errors are due to fluctuations in laser power; a variable which has not been considered in the uncertainty analysis. Variations, however, appear to be random and are expected to average out in the curve fitting process.
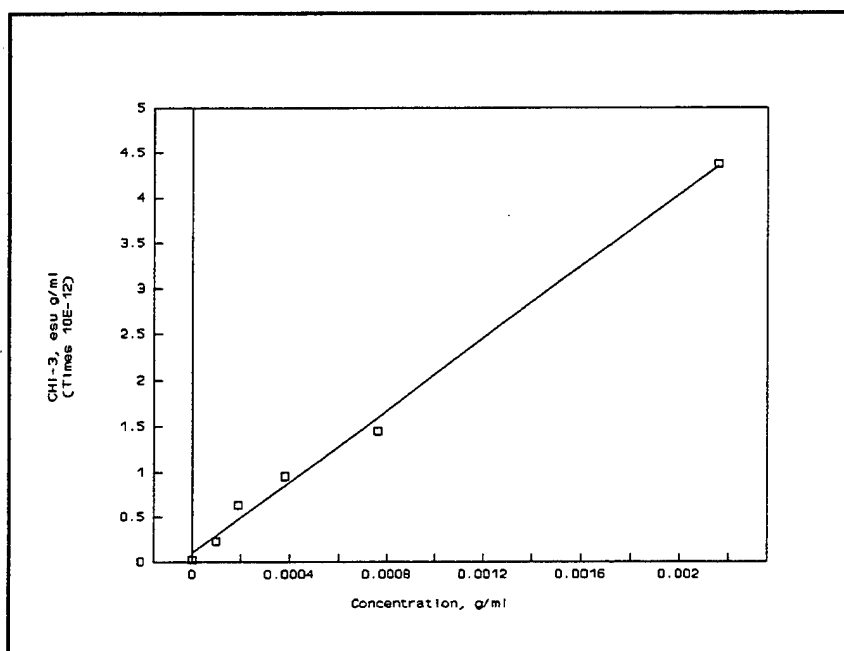
**Fig. 3.** Experimental data and curve-fit line versus concentration for zinc tetraphenyl tetrabenzporphyrin in tetrahydrafuran.

Table 5. Comparison of experimental and curve-fit data for zinc tetraphenyl tetrabenzporphyrin in tetrahydrafuran.

| $c$ (g/mL) | Experimental $\chi^{(3)}_{solution}$ ($\times 10^{-13}$ esu) | Curve-Fit $\chi^{(3)}_{solution}$ ($\times 10^{-13}$ esu) | Percent Error |
|---|---|---|---|
| 0.00216 | 43.7 | 43 | 2% |
| 0.00076 | 14.5 | 15 | 4% |
| 0.00038 | 9.57 | 7.8 | 23% |
| 0.00019 | 6.34 | 4.0 | 57% |
| 0.00010 | 2.31 | 2.2 | 5% |
| 0 | 0.24 | 0.24 | 0% |

## CONCLUSIONS AND RECOMMENDATIONS

Uncertainty expressions have been derived and used to evaluate a DFWM scheme used in the determination of third-order susceptibility and molecular second hyperpolarizability of nonlinear optical materials.

The results of a representative experimental run are presented showing that, for samples in solution, the greatest uncertainty is currently introduced by phase-conjugate voltage readings. As the strength of the phase-conjugate signal decreases, the overall experimental uncertainty increases. This relationship can occur as a result of a low laser output intensity or by the nonlinear material having a low phase-conjugate signal strength. Maximum experimental accuracy can be assured with proper laser maintenance and system alignment to optimize laser energy output and phase-conjugate signal strength.

Parameter sensitivity curves reveal that the indices of refraction of both the sample in solution and reference solution are the most critical parameters with respect to overall experimental uncertainty. Solution refractive indices are currently assumed equal to those of the solution solvent; the validity of this assumption should be verified in light of the results of this study.

Sensitivity plots contained in this report can be used as a general guide in estimating the impact of changes in tolerances of experimental variables. Accompanying software is now routinely used in DFWM experiments in determining $\chi^{(3)}$ and $\langle \gamma \rangle$ and their associated uncertainties.

Actual experimental deviations from a least-squares curve were shown to be within predicted uncertainties with the exception of some outliers attributable to variation in laser output power, which was not considered in the analysis.

Concerning the investigation of trends: results show that changes of $\pm 10\%$ percent or greater in $\chi^{(3)}$ and $\langle \gamma \rangle$ can be considered statistically significant. This confidence interval can be decreased by increasing the number of points (concentrations) used in the least-squares approximation.

The method of determining solution concentration outlined here has proven to be of acceptable accuracy ($\pm 1.6\%$) while also minimizing the production of hazardous waste and the time required to complete an experimental run.

It is believed that this study has given significant insight into the experimental uncertainties inherent to the DFWM technique when used in the evaluation of third-order susceptibility and molecular second hyperpolarizability of nonlinear optical materials.

# REFERENCES

1.  Rao, D.V.G.L.N., Aranda, F.J., Roach, J.F., Remy, D.E., *Appl. Phys. Lett.*, 1991, 58, 1241–1243.

## APPENDICES

A. Derivation of Mass/Concentration Expression
B. Computer Program ERRCHI-3.BAS
C. Parameter Sensitivity Curves

# APPENDIX A.  Derivation of Mass/Concentration Expression

A technique has been developed to determine dilute solution concentrations from accurate weight measurements.  The derivation is as follows:

An initial predetermined concentration $C_i$ is prepared of weight $m_i$ and density $\rho$.  Some solution is removed for measurement and the sample is weighed again. This final weight is $m_f$.  To determine the final volume $V_f$ we can write:

$$V_f = \frac{m_f}{\rho}.\qquad\text{(A1)}$$

The mass of the solute contained in $V_f$ can be determined by the expression

$$m_{solute} = C_i V_f.\qquad\text{(A2)}$$

Some solvent is added to dilute the solution for the next measurement.  This new, added volume can be obtained by the expression

$$V_+ = \frac{m_n - m_f}{\rho}.\qquad\text{(A3)}$$

The new concentration is

$$C_n = \frac{m_{solute}}{V_f + V_+}.\qquad\text{(A4)}$$

Inserting Eqs. A1, A2 and A3 into Eq. A4, we obtain the expression

$$C_n = \frac{C_i \frac{m_f}{\rho}}{\frac{m_f}{\rho} + \frac{m_n - m_f}{\rho}},\qquad\text{(A5)}$$

which reduces to

$$C_n = C_i \frac{m_f}{m_n}.\qquad\text{(A5)}$$

```
10    REM   This program calculates CHI-3 and Gamma for samples in solution.
20    REM   It can be used in conjunction with Lotus spreadsheet CHI-3.WK1
30    REM   which uses a least-squares curve-fitting routine to determine
40    REM   solute CHI-3 values from solution CHI-3 values calculated
50    REM   with this program.   B. Kimball,  18 March 1994.
60
70    CLS
100   INPUT "I of solution (mv) = ", Isol
110   INPUT "I of CS2, (mv) = ", Ics
120   REM Ics = 50000
130   INPUT "Absorbance, = ", ab
140   INPUT "Concentration, (mg/ml) = ", con
143
144   REM                     PARAMETERS FOR CHI-3 AND GAMMA EVALUATION

145   REM   Index of refraction of solution
147   ns = 1.44
150   REM   Path Length CS-2, (mm)
155   DCS = 2
160   REM   Path length solution, (mm)
162   DS = 2
165   REM   CHI-3 of Solvent, (esu)
167   Xsolv = 2.4E-14
168   REM   Uncertainty in Solvent CHI-3
170   WXsolv = 9.7E-16
172   REM   CHI-3 of CS-2
174   XCS = 6.8E-13
175   REM   Index of refraction of CS-2
180   ncs = 1.63
182   REM   Molecular weight of solute, g/mole
184   M = 678
186   REM   Avogadros number
188   A = 6.023E+23
190   REM   Mass of sample (mg)
195   mg = 3.8
200   REM   Volume of Solvent used in solution
205   ml = 5

210   REM                     PARAMETERS FOR CHI-3 UNCERTAINTY

220   PWXCS = 0
230   WXcs = XCS * PWXCS
240   PWIsol = .05
250   WIsol = Isol * PWIsol
260   PWIcs = .05
270   WIcs = Ics * PWIcs
280   PWns = .01
290   Wns = ns * PWns
300   PWncs = .001
310   Wncs = ncs * PWncs
320   PWDS = .001
330   WDS = DS * PWDS
340   PWDCS = .001
350   WDCS = DCS * PWDCS
360   PWab = .0008
370   Wab = ab * PWab
380   PWM = .001
390   WM = M * PWM
392   PWmg = .01
```

```
394   Wmg = mg * PWmg
396   PWml = .01
398   Wml = ml * PWml


400   REM                     CALCULATE CHI-3 AND GAMMA

405   alpha = -LOG(10 ^ -ab)
410   P1 = Isol / Ics
420   P2 = ns / ncs
430   P3 = DCS / DS
440   P4 = (alpha / (1 - (EXP(-alpha)))) * EXP(alpha / 2)
450   Xsol = XCS * (P1 ^ .5) * (P2 ^ 2) * P3 * P4
460   Xsam = (Xsol - Xsolv) / (con / 1000)
470   L = (ns ^ 2 + 2) / 3
480   GAMMA = (Xsam * M) / (L ^ 4 * A)


490   REM                     CALCULATE  Xsol UNCERTAINTY

495   REM    Sensitivity Expressions
500   SXcs = (P1 ^ .5) * (P2 ^ 2) * P3 * P4
510   SIsol = XCS * .5 * ((Isol ^ .5) ^ -1) * ((Ics ^ .5) ^ -1) *
         P2 ^ 2 * P3 * P4
520   SIcs = XCS * .5 * ((Isol ^ .5) / (Ics ^ 1.5)) * P2 ^ 2 * P3 * P4
530   Sns = XCS * (P1 ^ .5) * 2 * (ns / (ncs ^ 2)) * P3 * P4
540   Sncs = XCS * (P1 ^ .5) * ns ^ 2 * (2 / (ncs ^ 3)) * P3 * P4
550   SDCS = XCS * (P1 ^ .5) * (P2 ^ 2) * (1 / DS) * P4
560   SDS = XCS * (P1 ^ .5) * (P2 ^ 2) * (DCS / (DS ^ 2)) * P4
570   Sab = XCS * (P1 ^ .5) * P2 ^ 2 * P3 * ((1 - EXP(-alpha)) * ((alpha / 2) +
         EXP(alpha / 2)) - alpha * EXP(-alpha / 2)) / ((1 - EXP(-alpha)) ^ 2)

580   REM    Parameter Uncertainties
590   UXcs = SXcs * WXcs
600   UIsol = SIsol * WIsol
610   UIcs = SIcs * WIcs
620   Uns = Sns * Wns
630   Uncs = Sncs * Wncs
640   UDCS = SDCS * WDCS
650   UDS = SDS * WDS
660   Uab = Sab * Wab

670   REM Xsol Uncertainty
680   WXsol = (UXcs ^ 2 + UIsol ^ 2 + UIcs ^ 2 + Uns ^ 2 + Uncs ^ 2 +
         UDCS ^ 2 + UDS ^ 2 + Uab ^ 2) ^ .5


700   REM                     CALCULATE con UNCERTAINTY

710   REM    Sensitivity Expressions
720   Smg = 1 / ml
730   Sml = mg / (ml ^ 2)

740   REM Parameter Uncertainties
750   Umg = Smg * Wmg
760   Uml = Sml * Wml

770   REM  con Uncertainty
780   Wcon = (Umg ^ 2 + Uml ^ 2) ^ .5
```

```
800  REM              CALCULATE Xsam UNCERTAINTIES

810  REM   Sensitivity Expressions
820  SXsol = 1000 / con
830  SXsolv = 1000 / con
840  Scon = 1000 * (Xsol - Xsolv) / (con ^ 2)

850  REM   Parameter Uncertainties
860  UXsol = SXsol * WXsol
870  UXsolv = SXsolv * WXsolv
880  Ucon = Scon * Wcon

890  REM   Xsam Uncertainty
900  WXsam = (UXsol ^ 2 + UXsolv ^ 2 + Ucon ^ 2) ^ .5


950  REM              CALCULATE L UNCERTAINTIES

960  REM   Sensitivity Expressions
970  SLn = 2 * ns / 3

980  REM   Parameter Uncertainties
990  ULn = SLn * Wns

1000 REM   L Uncertainty
1010 WL = ULn


1020 REM              CALCULATE GAMMA UNCERTAINTIES

1030 REM   Sensitivity Expressions
1040 SXsam = M / ((L ^ 4) * A)
1050 SM = Xsam / ((L ^ 4) * A)
1060 SL = 4 * Xsam * M / ((L ^ 5) * A)

1070 REM   Parameter Uncertainties
1080 UXsam = SXsam * WXsam
1090 UM = SM * WM
1100 UL = SL * WL

1110 REM   GAMMA Uncertainty
1120 WGAMMA = (UXsam ^ 2 + UM ^ 2 + UL ^ 2) ^ .5


1200 REM                    PRINT RESULTS

1204 PRINT "                    RESULTS"
1205 PRINT
1210 PRINT "CHI-3 of solution is"; Xsol
1220 PRINT "Uncertainty"; WXsol
1230 PRINT
1240 PRINT "CHI-3 of sample is"; Xsam
1250 PRINT "Uncertainty"; WXsam
1260 PRINT
1270 PRINT "Gamma of the solute is"; GAMMA
1280 PRINT "Uncertainty"; WGAMMA
```

```
1310   PRINT "                    PARAMETER UNCERTAINTIES"
1320   PRINT
1330   PRINT "                           Xsol"
1340   PRINT "CHI-3 of CS2 "; UXcs
1350   PRINT "Voltage reading for solution"; UIsol
1360   PRINT "Voltage reading for CS2"; UIcs
1370   PRINT "Solution refractive index"; Uns
1380   PRINT "CS2 refractive index"; Uncs
1390   PRINT "Solution thickness"; UDS
1400   PRINT "CS2 thickness"; UDCS
1410   PRINT "Absorption"; Uab
1415   INPUT ; "Hit Return", me
1416   CLS
1420   PRINT
1430   PRINT "                    Concentration"
1440   PRINT "Weight"; Umg
1450   PRINT "Volume"; Uml
1470   PRINT
1480   PRINT "                       Xsam"
1490   PRINT "Solution CHI-3"; UXsol
1500   PRINT "Solvent CHI-3"; UXsolv
1510   PRINT "Concentration"; Ucon
1520   PRINT
1530   PRINT "                    Field Factor L"
1540   PRINT "Solution refractive index"; ULn
1550   PRINT
1560   PRINT "                       GAMMA"
1570   PRINT "Sample CHI-3"; UXsam
1580   PRINT "Molecular weight"; UM
1590   PRINT "Field Factor L"; UL
1700   END
```

## APPENDIX C. Parameter Sensitivity Curves.
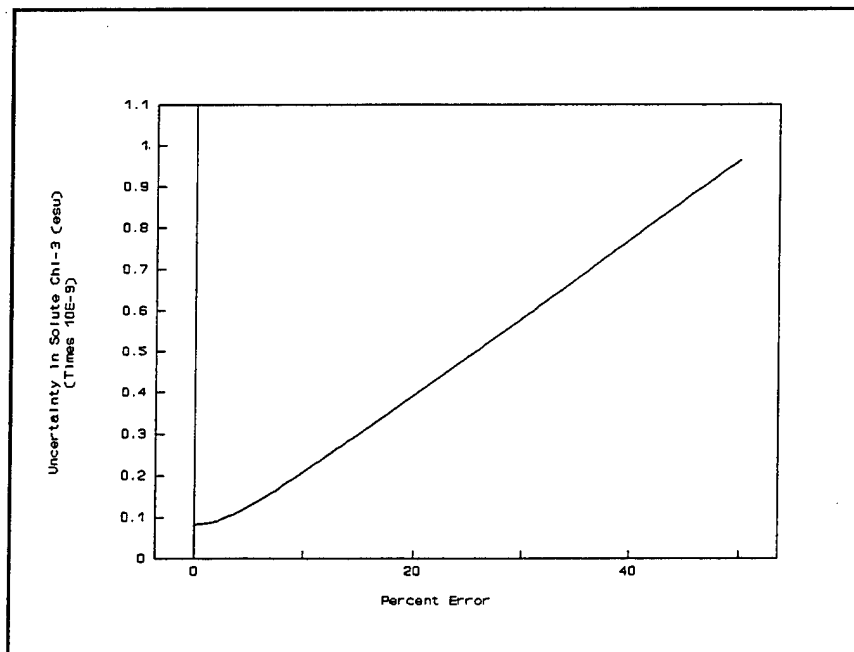


Fig. C1. Uncertainty in $\chi^{(3)}$ resulting from percent error in the assumed value for the $\chi^{(3)}$ of $CS_2$.
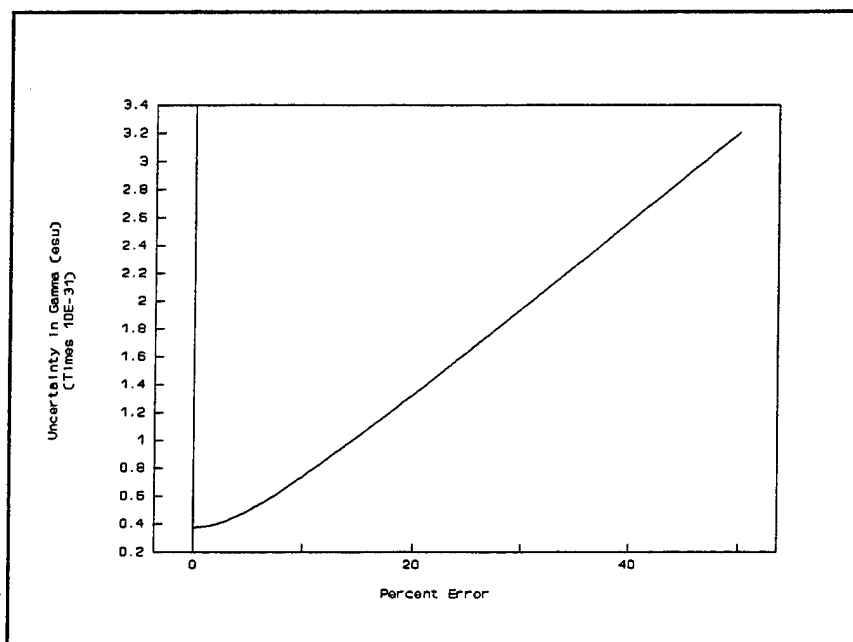


Fig. C2. Uncertainty in $\langle\gamma\rangle$ resulting from percent error in the assumed value for the $\chi^{(3)}$ of $CS_2$.
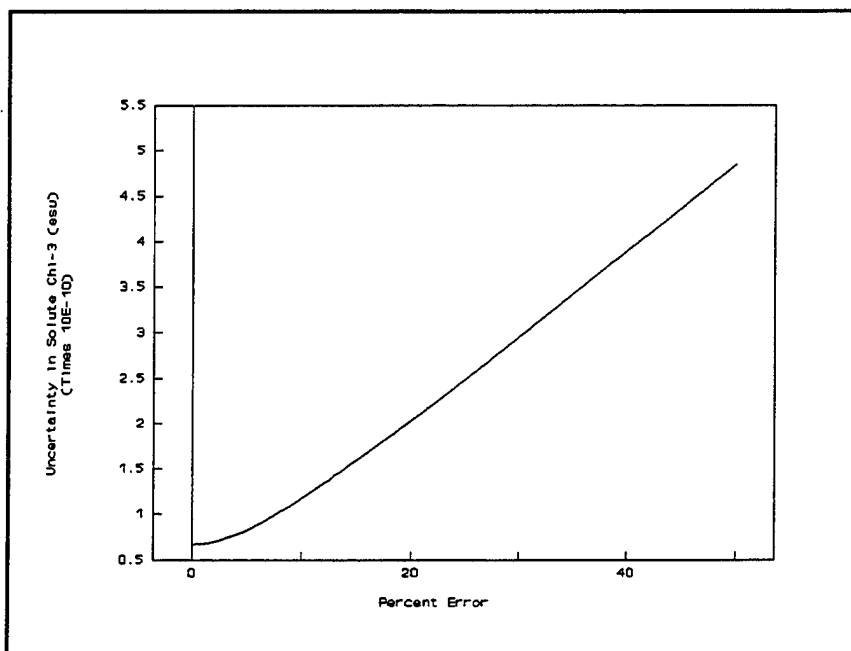
Fig. C3. Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in the DFWM phase-conjugate signal of the solution.
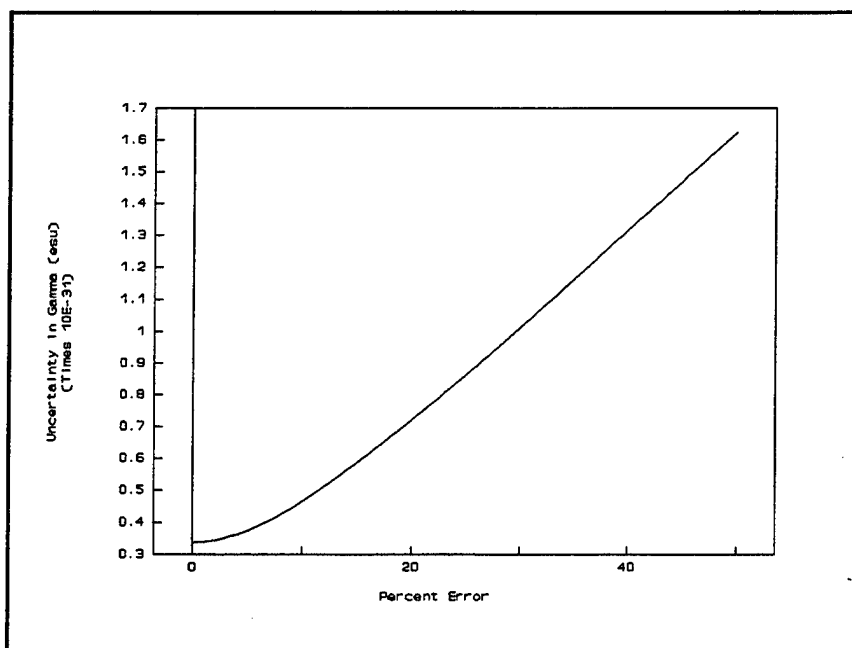


Fig. C4. Uncertainty in $\langle\gamma\rangle$ resulting from percent error in the DFWM phase-conjugate signal of the solution.
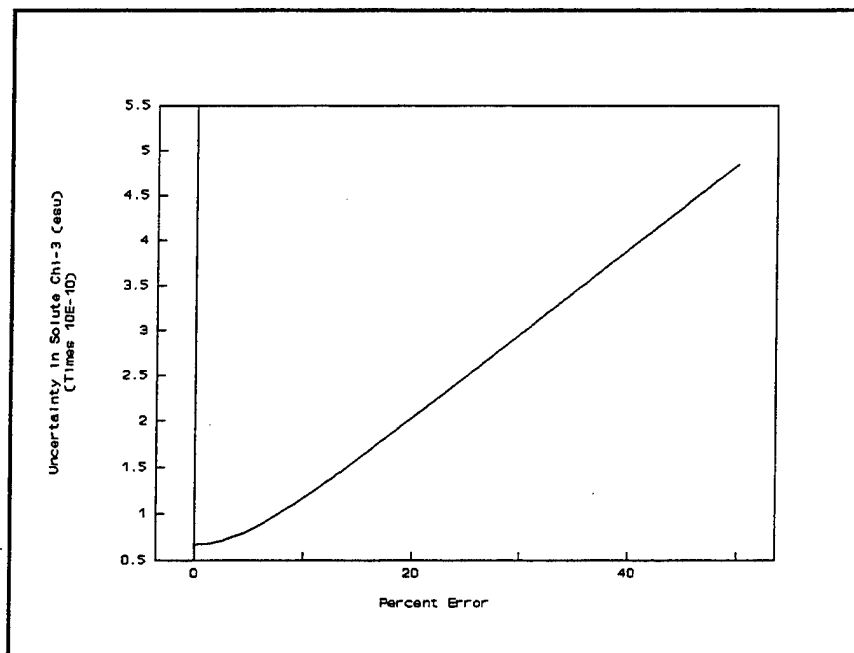
Fig. C5. Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in the DFWM phase-conjugate signal of $CS_2$.
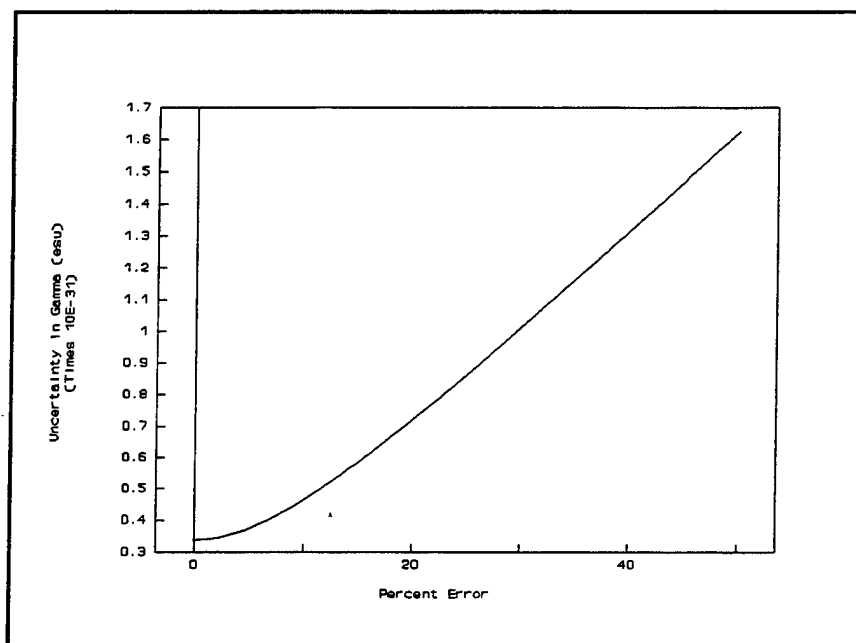


Fig. C6. Uncertainty in $\langle\gamma\rangle$ resulting from percent error in the DFWM phase-conjugate signal of $CS_2$.
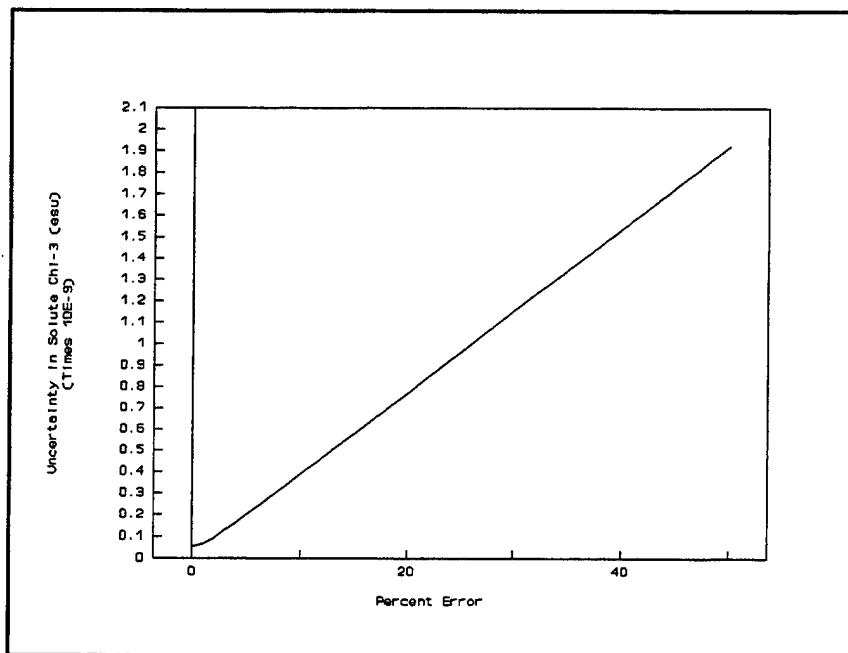
Fig. C7.   Uncertainty in $\chi^{(3)}{}_{solute}$ resulting from percent error in
the index of refraction of the solution.
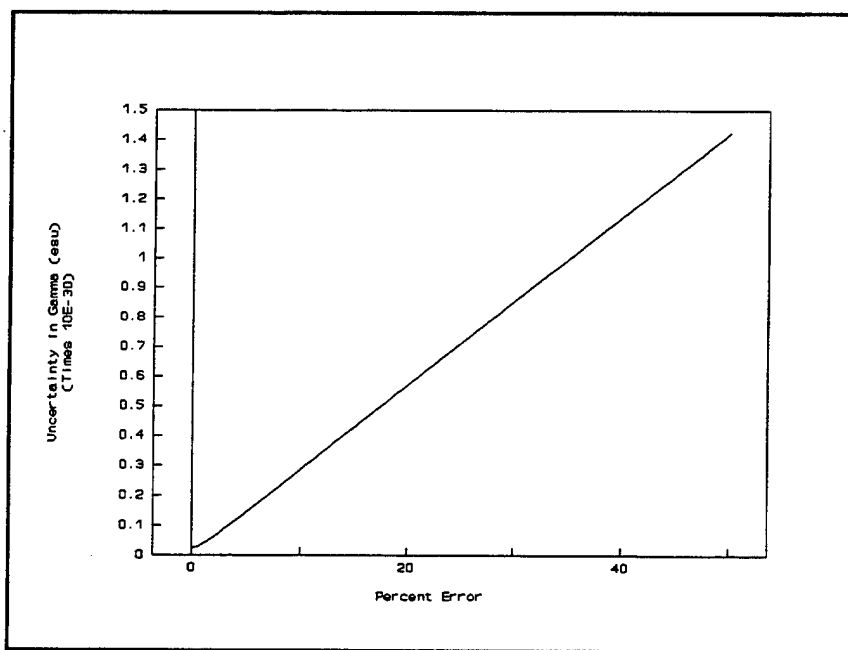


Fig. C8.   Uncertainty in $\langle \gamma \rangle$ resulting from percent error in
the index of refraction of the solution.

27
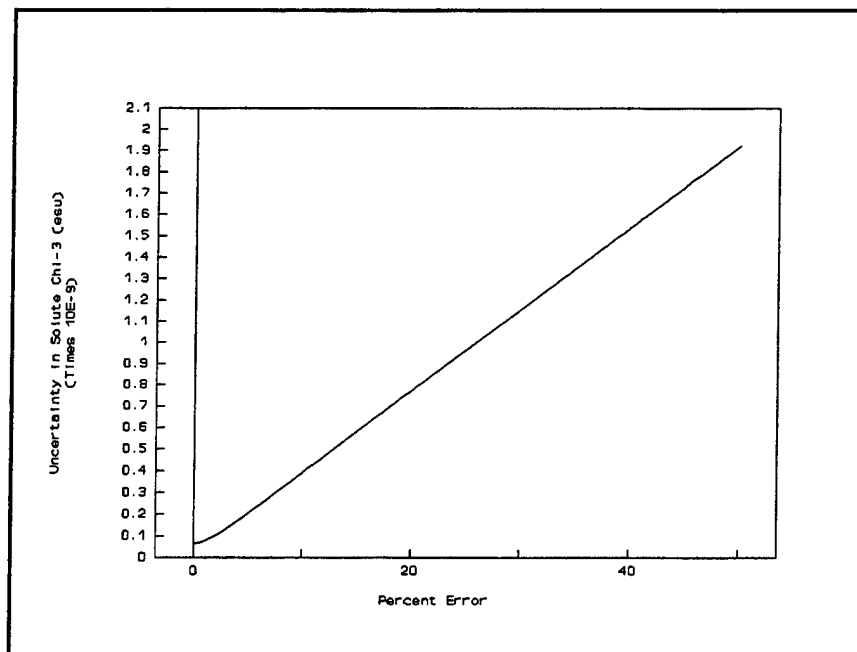
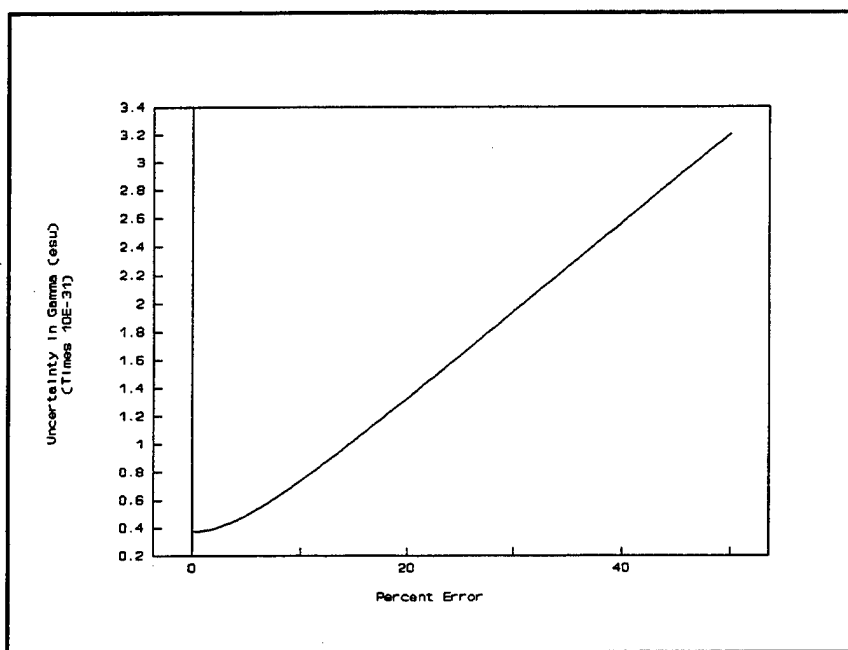Fig. C9. Uncertainty in $\chi^{(3)}_{\text{solute}}$ resulting from percent error in the index of refraction of $CS_2$.
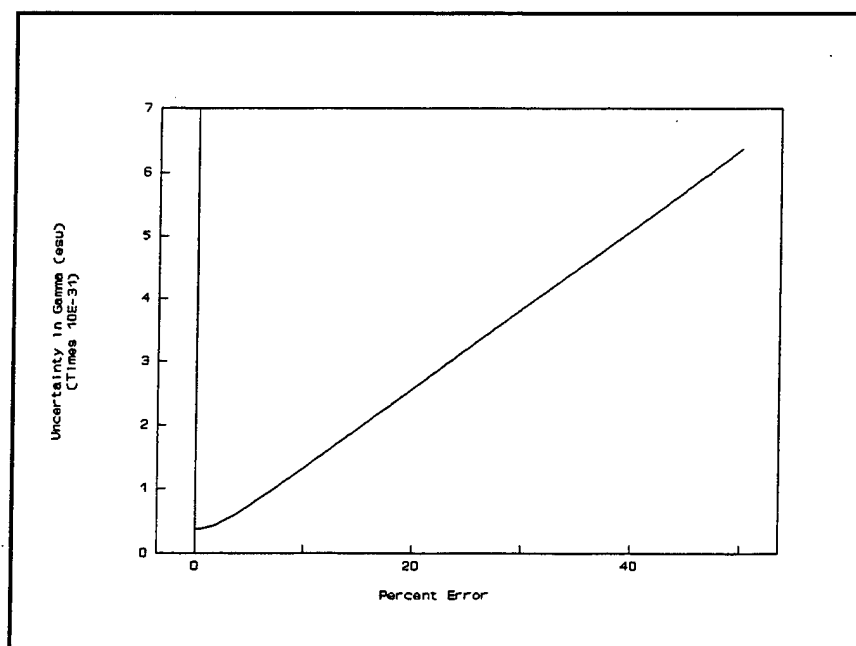


Fig. C10. Uncertainty in $\langle \gamma \rangle$ resulting from percent error in the index of refraction of $CS_2$.
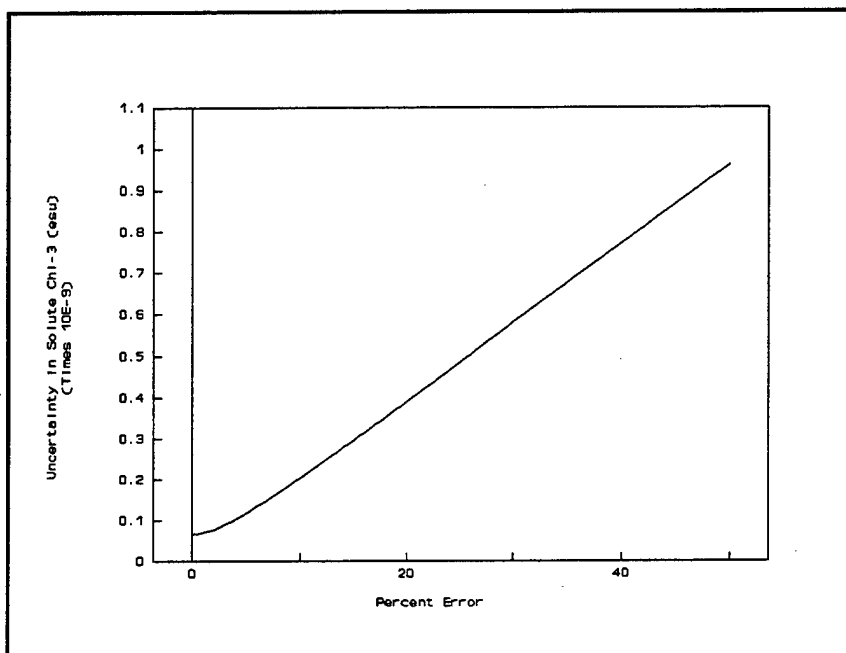
Fig. C11.   Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in sample thickness.



Fig. C12.   Uncertainty in $\langle \gamma \rangle$ resulting from percent error in sample thickness.
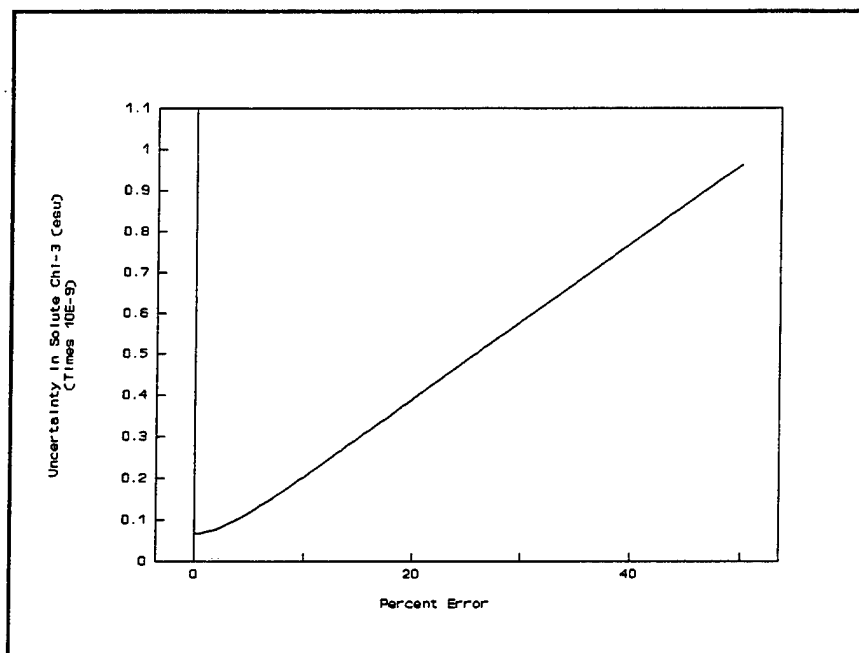
Fig. C13.   Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in CS$_2$ thickness.
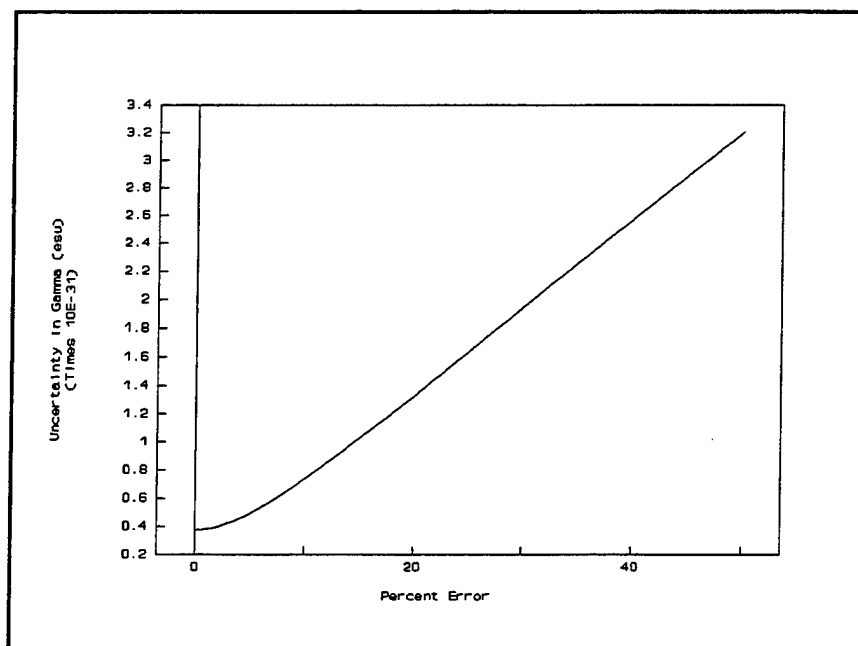


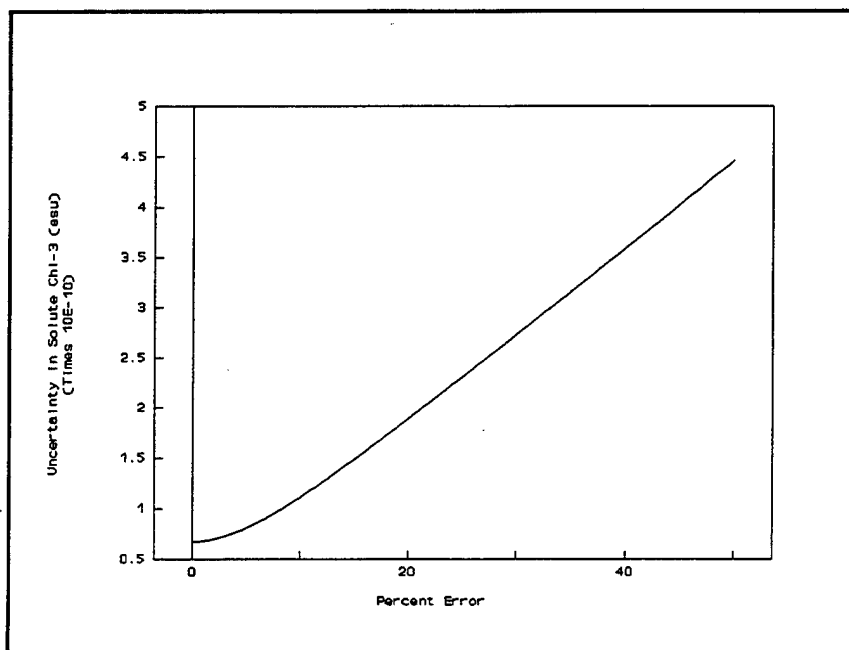Fig. C14.   Uncertainty in $\langle\gamma\rangle$ resulting from percent error in CS$_2$ thickness.

30

Fig. C15.   Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in sample absorption.
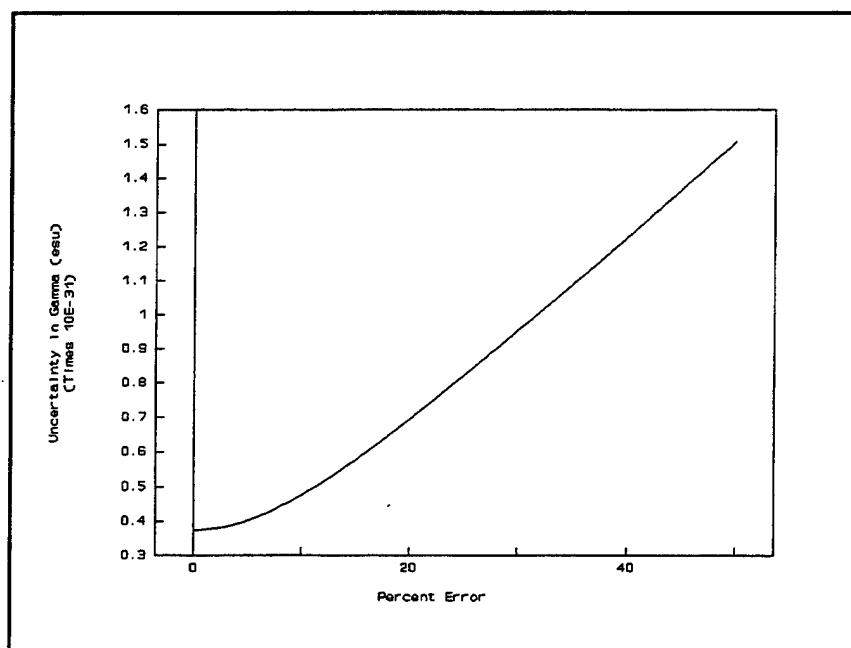


Fig. C16.   Uncertainty in $\langle \gamma \rangle$ resulting from percent error in sample absorption.
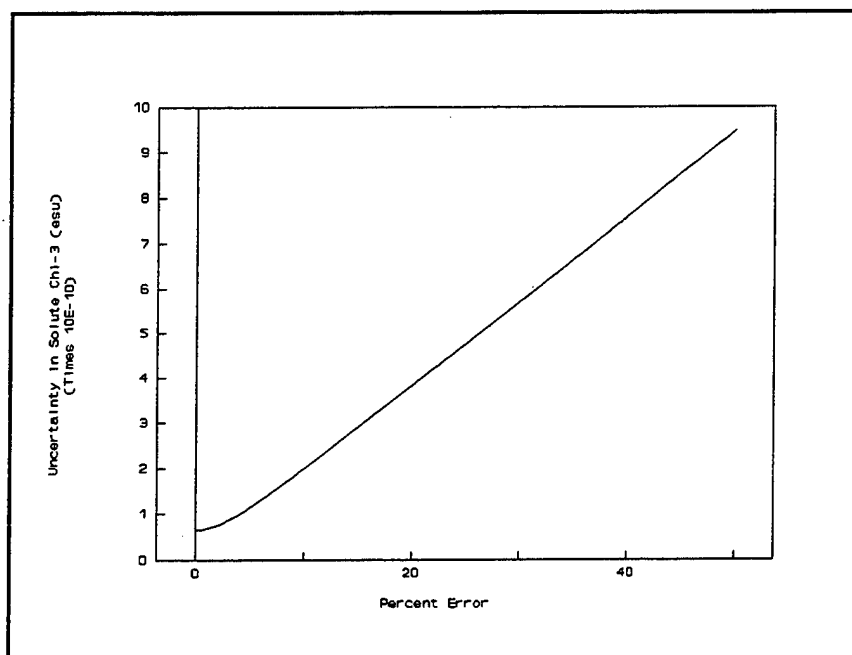
31

**Fig. C17.** Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in measurement of solution weight.
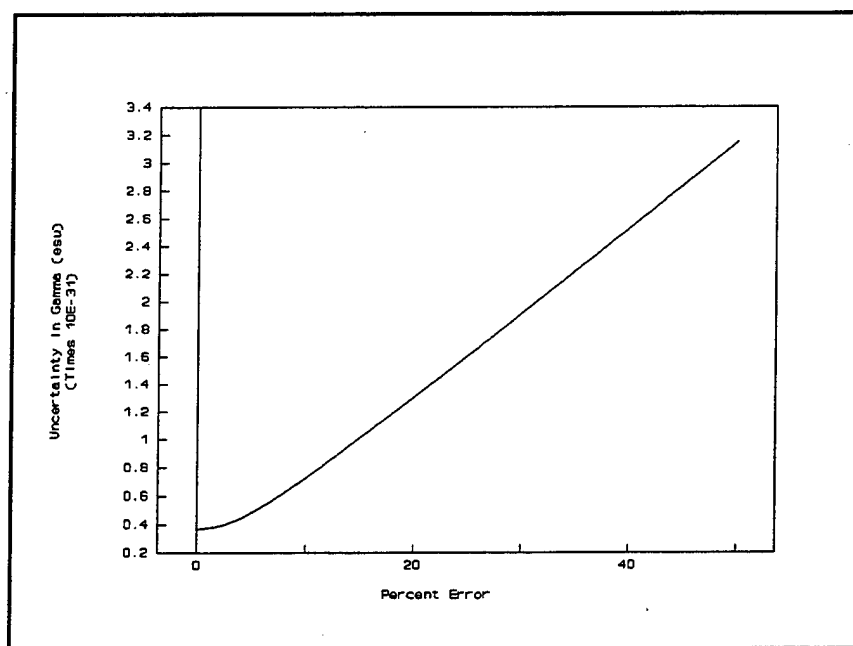


**Fig. C18.** Uncertainty in $\langle\gamma\rangle$ resulting from percent error in measurement of solution weight.
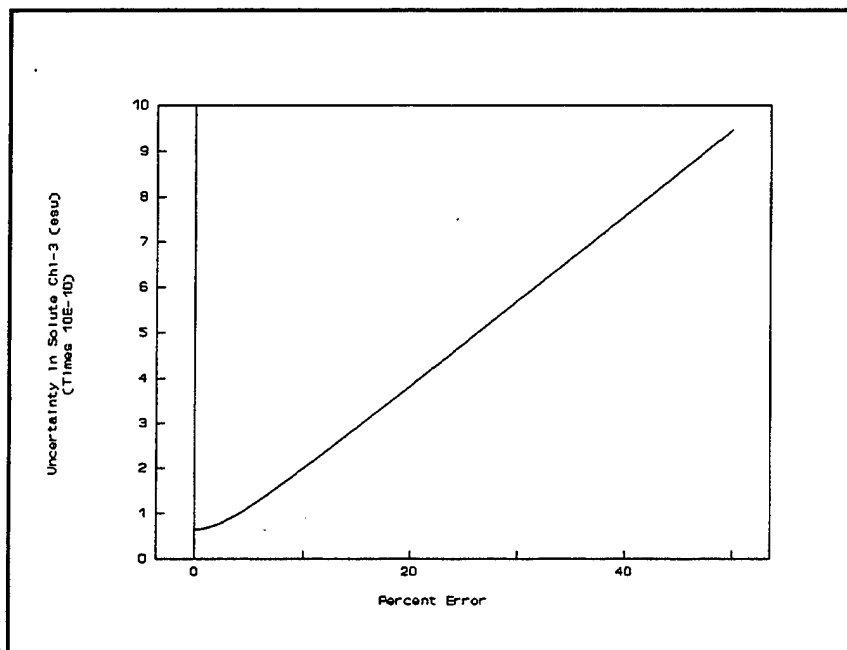
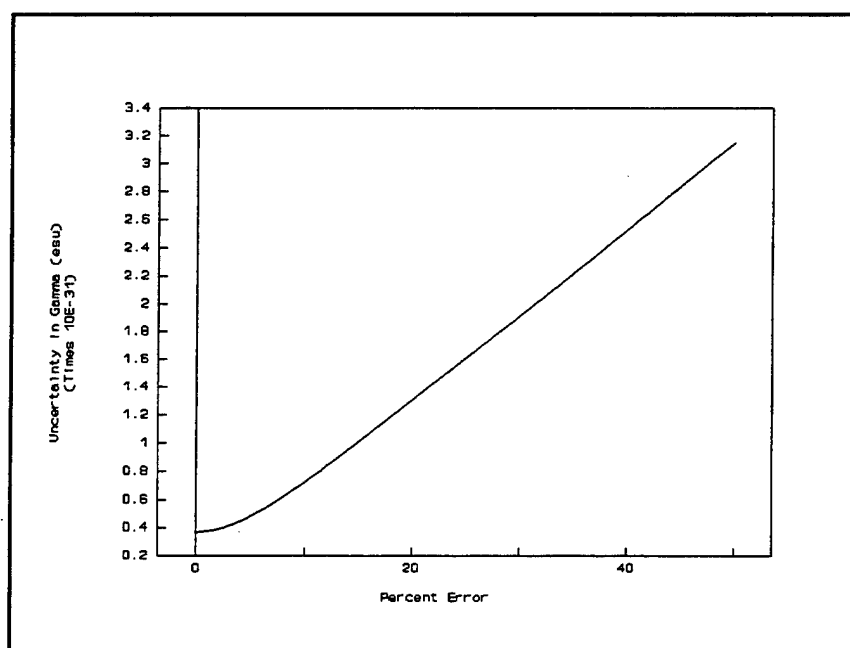Fig. C19. Uncertainty in $\chi^{(3)}_{solute}$ resulting from percent error in measurement of solution volume.



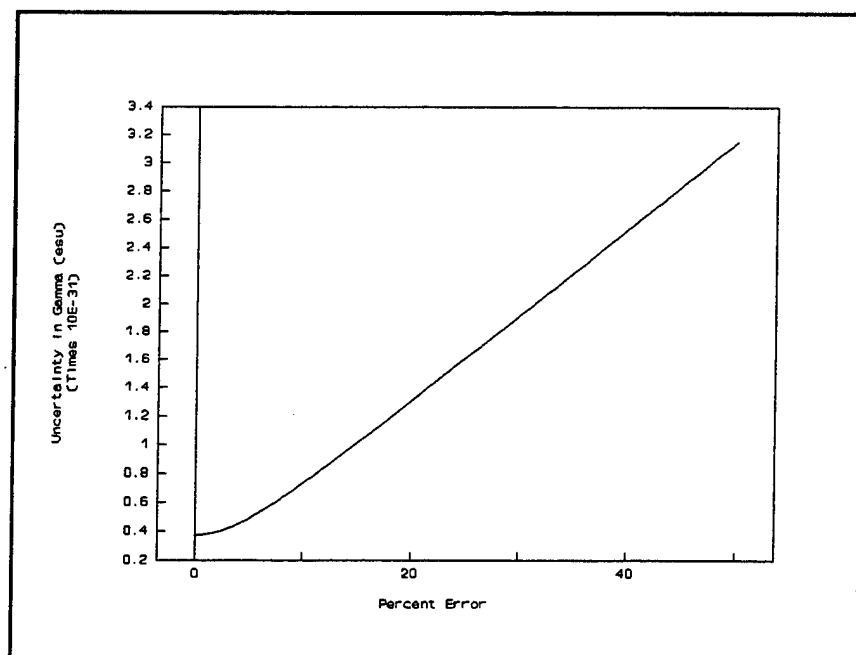Fig. C20. Uncertainty in $\langle\gamma\rangle$ resulting from percent error in measurement of solution volume.

Fig. C21.  Uncertainty in $\langle\gamma\rangle$ resulting from percent error in molecular weight of solute.

# DISTRIBUTION LIST

1 copy to:

    COMMANDER
    U.S. ARMY TRAINING AND DOCTRINE
    COMMAND
    ATTN: ATCD-SE
    FT. MONROE, VA  23651

1 copy to:

    PROGRAM MANAGER - CLOTHING AND
    INDIVIDUAL EQUIPMENT
    ATTN: AMCPM-CIE
    WOODBRIDGE, VA  22194-4206

1 copy to:

    COMMANDANT
    U.S. ARMY INFANTRY SCHOOL
    ATTN: ATSH-CD-MLS-C
    FT. BENNING, GA  31905

1 copy to:

    COMMANDANT
    U.S. ARMY ARMOR SCHOOL
    ATTN: ATSB-CD-ML
    FT. KNOX, KY  40121-5215

1 copy to:

    COMMANDANT
    U.S. ARMY CHEMICAL SCHOOL
    ATTN: ATZN-CM-CS
    FT. McCLELLAN, AL  36205-5000

1 copy to:

    COMMANDANT
    U.S. ARMY AVIATION SCHOOL
    ATTN: ATZQ-CDM-C
    FT. RUCKER, AL  36362

1 copy to:

    COMMANDER
    U.S. ARMY NUCLEAR AND
    CHEMICAL AGENCY
    ATTN: MONA-NU  BLDG. 2073
    7500 BACKLICK ROAD
    SPRINGFIELD, VA  22150-3198

1 copy to:

COMMANDER
U.S. ARMY NUCLEAR AND
CHEMICAL AGENCY
ATTN: MONA-ZB BLDG.2073
7500 BACKLICK ROAD
SPRINGFIELD, VA 22150-3198


1 copy to:

DIRECTOR
DEFENSE NUCLEAR AGENCY
ATTN: TDTR
6801 TELEGRAPH ROAD
ALEXANDRIA, VA 23310-3398


1 copy to:

DIRECTOR
DEFENSE NUCLEAR AGENCY
ATTN: HRP
6801 TELEGRAPH ROAD
ALEXANDRIA, VA 23310-3398


1 copy to:

HQDA
OFFICE OF THE SURGEON GENERAL
ATTN: DASG-HCG
5109 LEESBURG PIKE
FALLS CHURCH, VA 22041-3258


1 copy to:

COMMANDER
U. S. ARMY COMBINED ARMS DEFENDE CENTER
ATTN: ATZL-CAD-N
FT. LEAVENWORTH,KS 66027-5300


1 copy to:

U.S. ARMY AVIATION MEDICAL RESEARCH
LABORATORY
ATTN: SGRD-VAB-CB
FT. RUCKER, AL 36352-5000


1 copy to:

COMMANDER
WALTER REED INSTITUTE OF RESEARCH
ATTN: SGRD-UWZ
WASHINGTON, DC 20307-5100


1 copy to:

U.S. ARMY RESEARCH LABORATORY
ATTN: SLCHD-NW-TN
2800 POWDER MILL ROAD
ADELPHI, MD 20783

1 copy to:

U.S. NAVY CLOTHING AND TEXTILE
RESEARCH FACILITY
ATTN:  CODE 40.1
21 STRATHMORE ROAD
NATICK, MA   01760-2490


2 copies to:

DEFENSE TECHNICAL INFORMATION CENTER
CAMERON STATION
ALEXANDRIA, VA   22314


7 copies to:

COMMANDER
U.S. ARMY NATICK RD & E CENTER
TECHNICAL LIBRARY
ATTN:  STRNC-MIL
NATICK, MA   01760


1 copy to:

COMMANDER
U.S. ARMY NATICK RD & E CENTER
ATTN:  STRNC-MSR
NATICK, MA   01760-5020


50 copies to:

COMMANDER
U.S. ARMY NATICK RD & E CENTER
ATTN:  STRNC-YSD (Mr. Kimball)
NATICK, MA   01760-5020